

Application Note

The use of FlexyPAT-HFC for calorimetric measurements


Regardless if you need to do process safety measurements for scale-up studies, kinetic analysis for process optimization, etc., with FlexyPAT-HFC you have a strong and flexible tool in your laboratory.

FlexyPAT is a modular **P**rocess **A**utomation **T**echnology that enables automated customer-specific lab reactor systems to be implemented in a very cost-effective manner, including with the integration of existing devices.

The option "Heat-Flow-Calorimetry" converts, within a few minutes, a standard SYSTAG FlexyPAT system into a sophisticated Heat-Flow calorimeter. The design and performance of this easy-to-use calorimeter fulfills the basic requirements in typical R&D laboratories.

Performance

- ⇒ Isothermal Heat-Flow Calorimeter with optionally Heat-Balance for reflux-condenser.
- \Rightarrow Flexible system for different reactors from 500ml up to 5l, glass or steel vessels.
- \Rightarrow Intuitive Recipe Control Software allows changes "on-the-fly".
- ⇒ Integration of third-party technology like turbidity, FT-IR, particle-size analyzer, sampling Systems, ultrasonicators, etc.






Functionality

FlexyPAT is a flexible system, that allows customised functionality. The basic system includes:

- ⇒ Temperature control, jacket or reactor mode
- ⇒ Stirrer speed control and torque measurement
- ⇒ 2 dispensing (gravimetric or volumetric)
- ⇒ pH-control (pX-control)
- \Rightarrow Automatic distillation^[1] / pressure-vacuum control^[1] / hydrogenation^[1] / automatic solubility^[1]

The base of success

Apart from the standardised lab-glassware, the intuitive and user-friendly software is another productive features of FlexyPAT. Not only specialists but also newcomers in calorimetry will become familiar with this system within a short period of time! A key-figure of the word-wide success of all the SYSTAG applications is the very intuitive software.

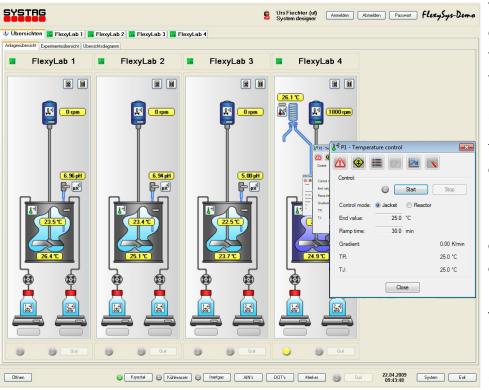

This picture shows the graphic interface of simultaneous reactor operations. Up to 6 reactors in parallel, each with 2 gravimetric feed can be controlled on 1 PC. (Here, 4 are shown.)

SYSTR

By manual operation every function (T-control, dosage, stirrer) is activated by a simple click on its symbol to open a sub-window with further parameters. Data logging & trending is possible at any time during the process.

^[1]optional



OperX - SYSTAG - C:\FlexySysV	rojectVRc:jpesVCU8_1283_Experiment1.sor
Elle Edit Yew 2	
	b P X 10 B k = 1 = = ●
Common	🖇 Franc 1 - Alam settings
Phase	Ensigency Alarm
Temperature (*	Upper Init TR 200 °C Upper Init TJ 200 °C
Temperature control	Upper link p 1.5 bar Adam 11 25 °C
Temperature parameters	Alam timer 200 rpm
Dosage 1 (R	S Phase 2 Temperature Control Reactor
Dosage 1	Reactor Control 🔒 Stimer on 200
Dosage 1 stop criteria	Control mode Reactor Speed setpoint 200 pm End value 190 °C Sincer same 12-400 pm
Dosage 1 pump	Rappine 45 min Differencial/Setu
Dosage 2 (*	Difference (TP-12) K High lead TR 200 °C
Start docage 2	Low first TR - 100 °C Batch mode Batch
Dosage 2 parameters	S Paur (Sublision
Dosage 2 stop criteria	-
	O Trace (v/at) Deby time 30 min
pX (R)	
pX pX control pX pX parameters	Phase 4 1st Addison (Methanol)
Pressue	Concept of Methanol Concept of Methanol Concept Descept D
	Ramp time 35 min Stimer range 12400 pm DOT 2 Off Stop ramp if pX < pX
Distillation (8)	Hold # dW > g Hold # dW > g Hold # dW > 5 K Hold # dX > gX
Stiner R	Balance mode Finance Batch mode Batch
Stiner	
Calorimetry ¥	Phase 5 Take sample (wat for end of reaction)
System (*	Control Control Showed text Tails sample Debu time 30 min
Digital outputs	
Alam 😵	S Pare 6 - Hydoleia
Logicals ¥	End value 200 g
Flag	Ramp time 10 min
Experiment 8	Hold # dox >
Capennar	Balance mode From balance Balance mode Balan
	Phase 7 Stabilization
	Detay line 80 min
	\$ Paul
40	24.3.2005 09.46.04

The included Batch-Recipe-Editor is based on "Drag & Drop" MS-Windows technology.

All existing operations (Temp, Dosage, Stirrer etc.) are listened in the table on the left side. A new recipe is created by drag & drop functionality.

Often used sequence of steps and operations may be stored as a "method" and can be added at any place in a recipe.

No better way to create SOP (Standard Operation Procedures)! Changes "on-the-fly" are possible, as well as manual interaction by the user. The report file recognizes all the events.

Calorimetric results


All SYSTAG calorimeters provide the following results:

- \Rightarrow Heat & power of reaction
- \Rightarrow Adiabatic temperature rise (MTSR)
- \Rightarrow Accumulation of reaction


In combination with the option "Heat Balance Calorimetry," the above mentioned results are given separately for the reflux condenser term for reaction at the boiling point.

All these results are not only given as numeric values but also displayed in a chart (see next page).

The isothermal heat-flow calorimetry is the most common technology for reaction calorimetry in Safety and R&D Laboratories.

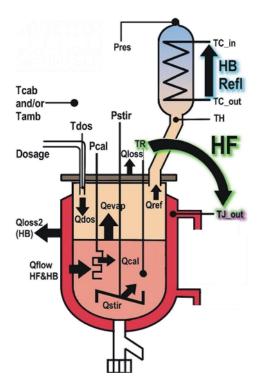



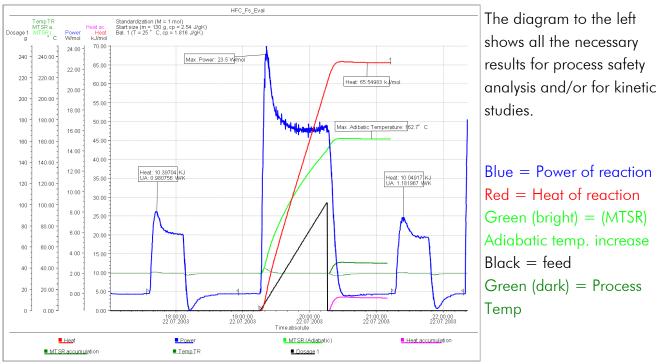


Power & Heat of Reaction: From the graph it is possible to read the maximum Power and Heat given by the reaction.

Adiabatic Temperature: The MTSR (maximum temperature by synthesis reaction) displays the worstcase for the present experiment. Assuming a cooling failure, the process temperature (35°C) could increase under adiabatic conditions up to about 160°C (green bright).

Accumulation: It is important to understand the accumulation of a Process. By the above shown graph, it is easy to distinguish between total heat (red) and accumulation (pink). The present experiment accumulates by about max. 10% (compare pink and red curve).

Run-away Reaction & Critical Class: Further analysis like Run-away Scenario or classification regarding the Critical Classes of reaction can be done, based on the above shown results.

SYSTAG supports you to evaluate the most relevant equipment for all your needs in the scope of Controlled Lab Reactors, Thermal Process Safety and Plant Control Systems.



Copyright SYSTAG AG, 2012